



Calibration CDN D100

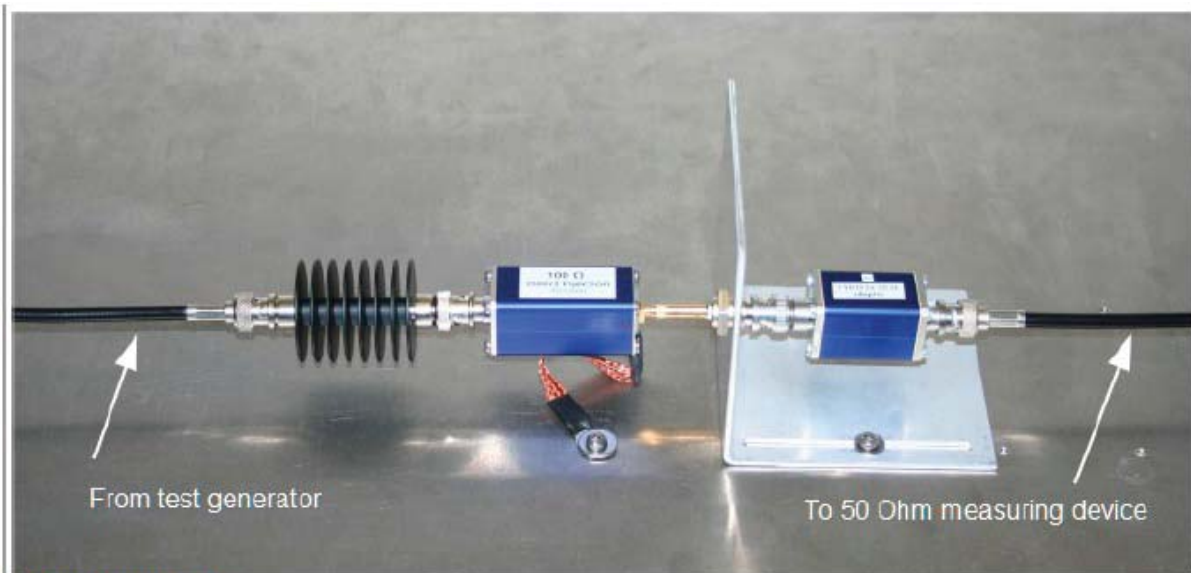

Setting of the output level

Network Analyser HP8751A (S.-No.: 3315J01756), Test Set 87512A (S.-No. MY43100614)
Common mode impedance, measurement method acc. IEC/EN61000-4-6
Direct coupling 100 Ohm

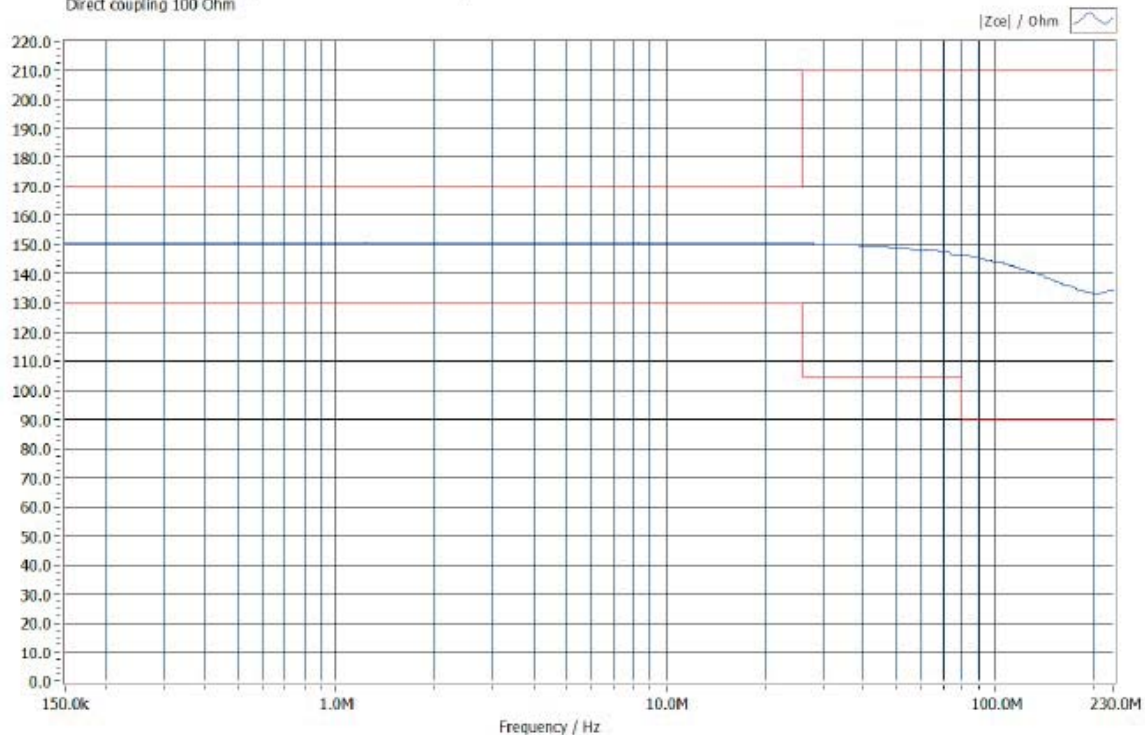

Typical common mode impedance