


CERTIFICATE OF CALIBRATION

Date: 1/6/2015
Model: 3525
Serial Number:

Temperature: 74 °F
Relative Humidity: 44 %

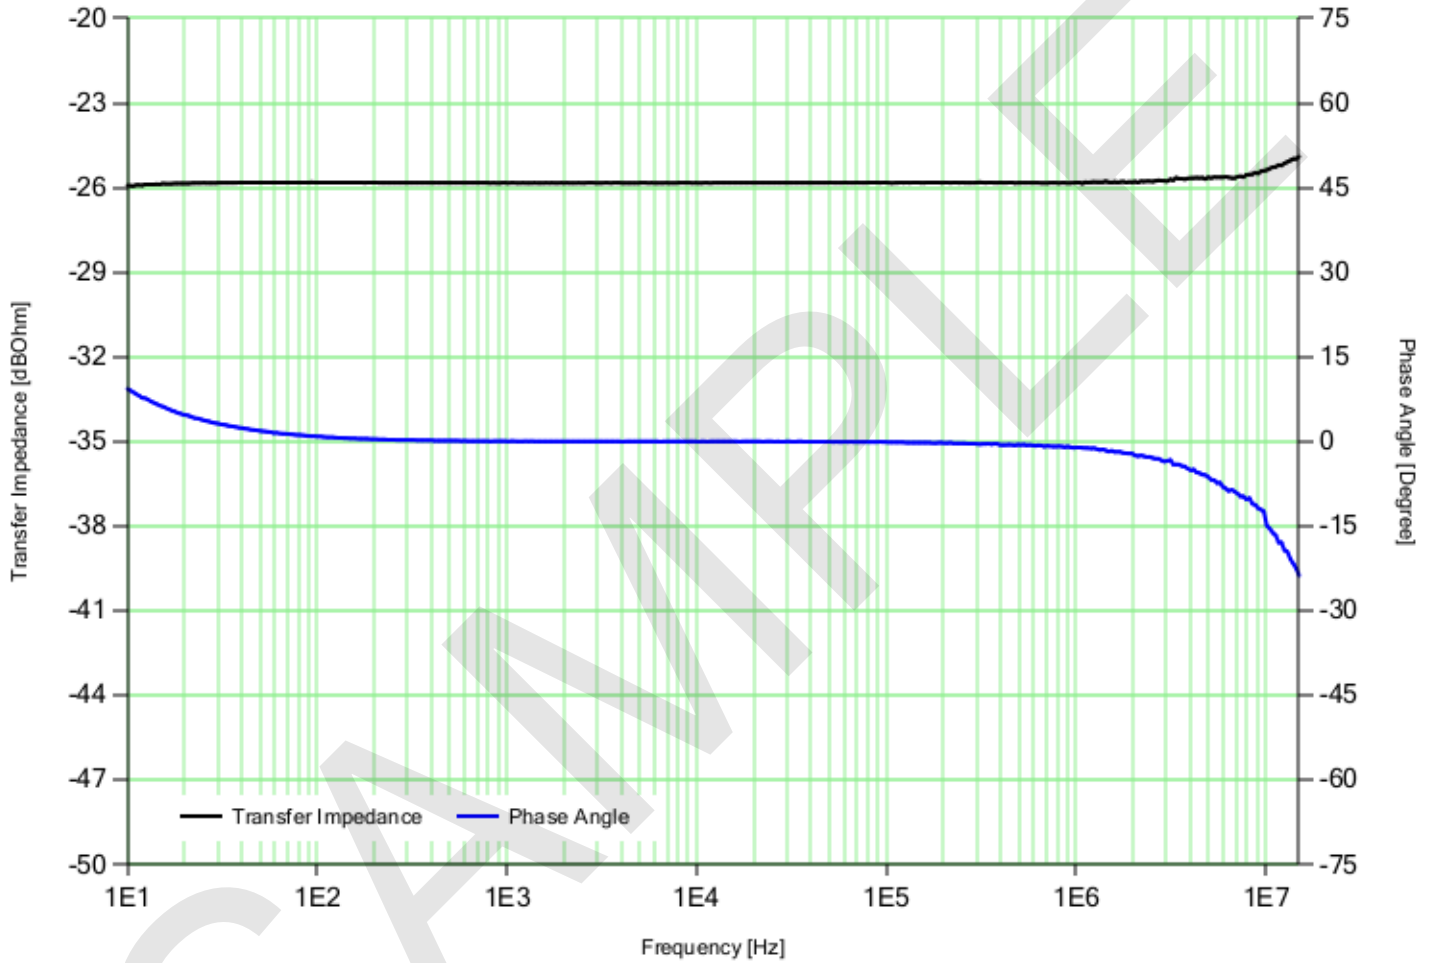

Nominal sensitivity 0.05(V/A) (-26 dBOhm)

The policies and procedures and this facility comply with ANSI/NCSL Z540-3 and ISO 9001:2008 and are traceable to NIST.

Calibration Equipment Used:	ID Number	Cal Date	Due Date
Model Type HP 4195A Network Analyzer	2830J00997	09-21-14	09-21-16

Certified By: _____